

1/5

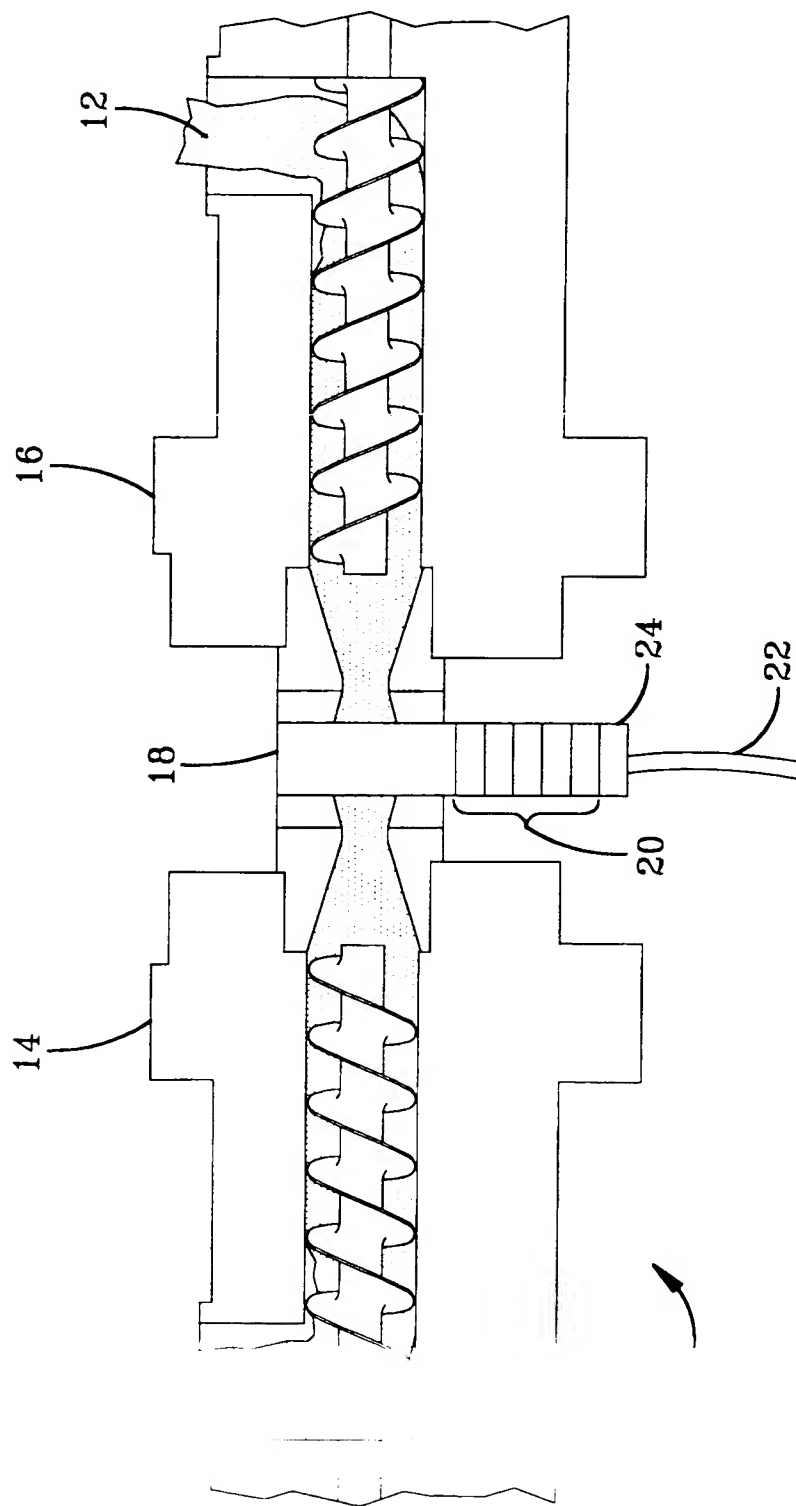


FIG-1

2/5

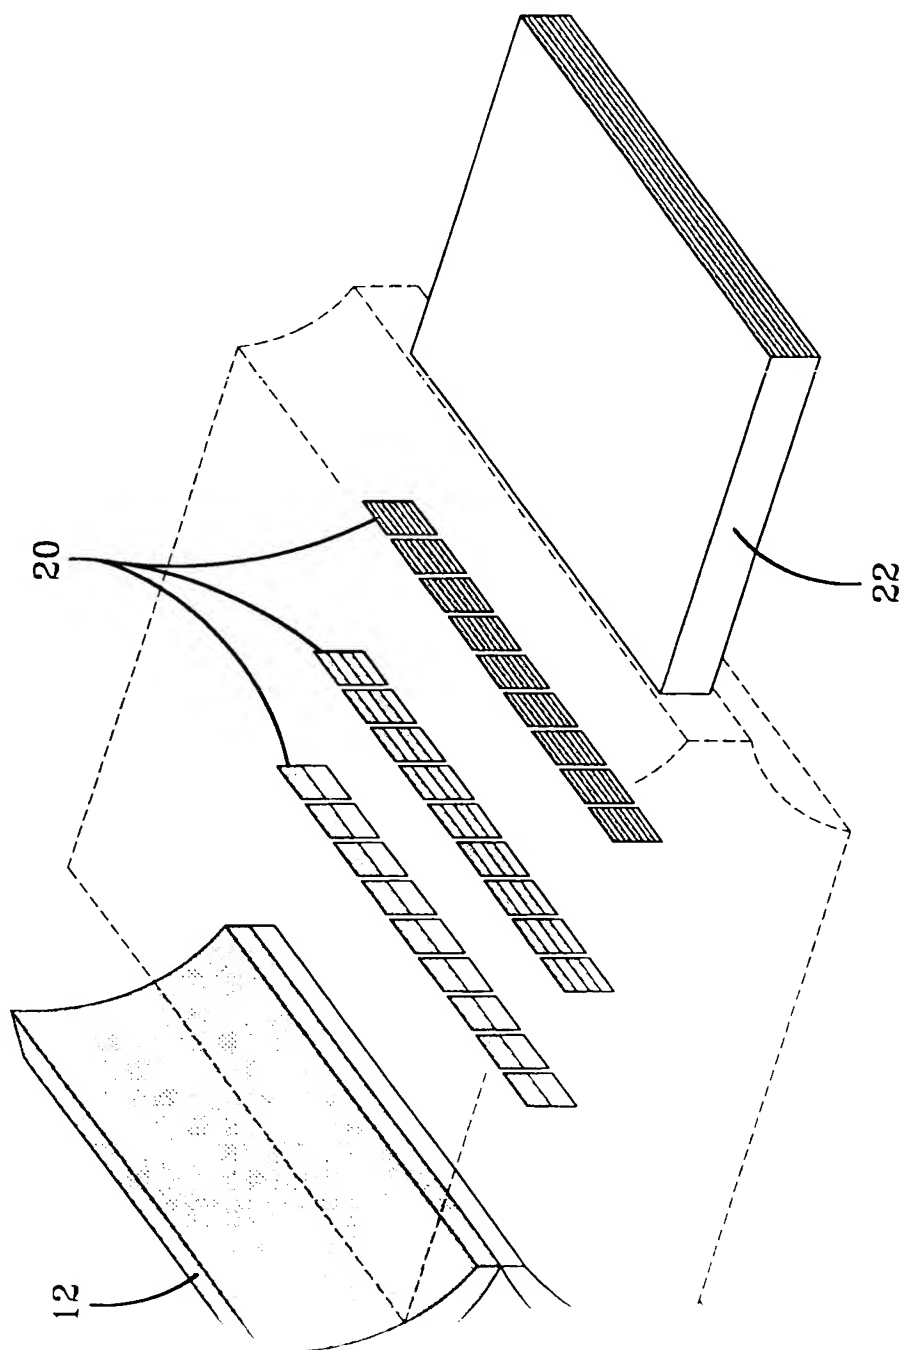


FIG-2

# MULTILAYER PROCESS AND DIE OPERATION

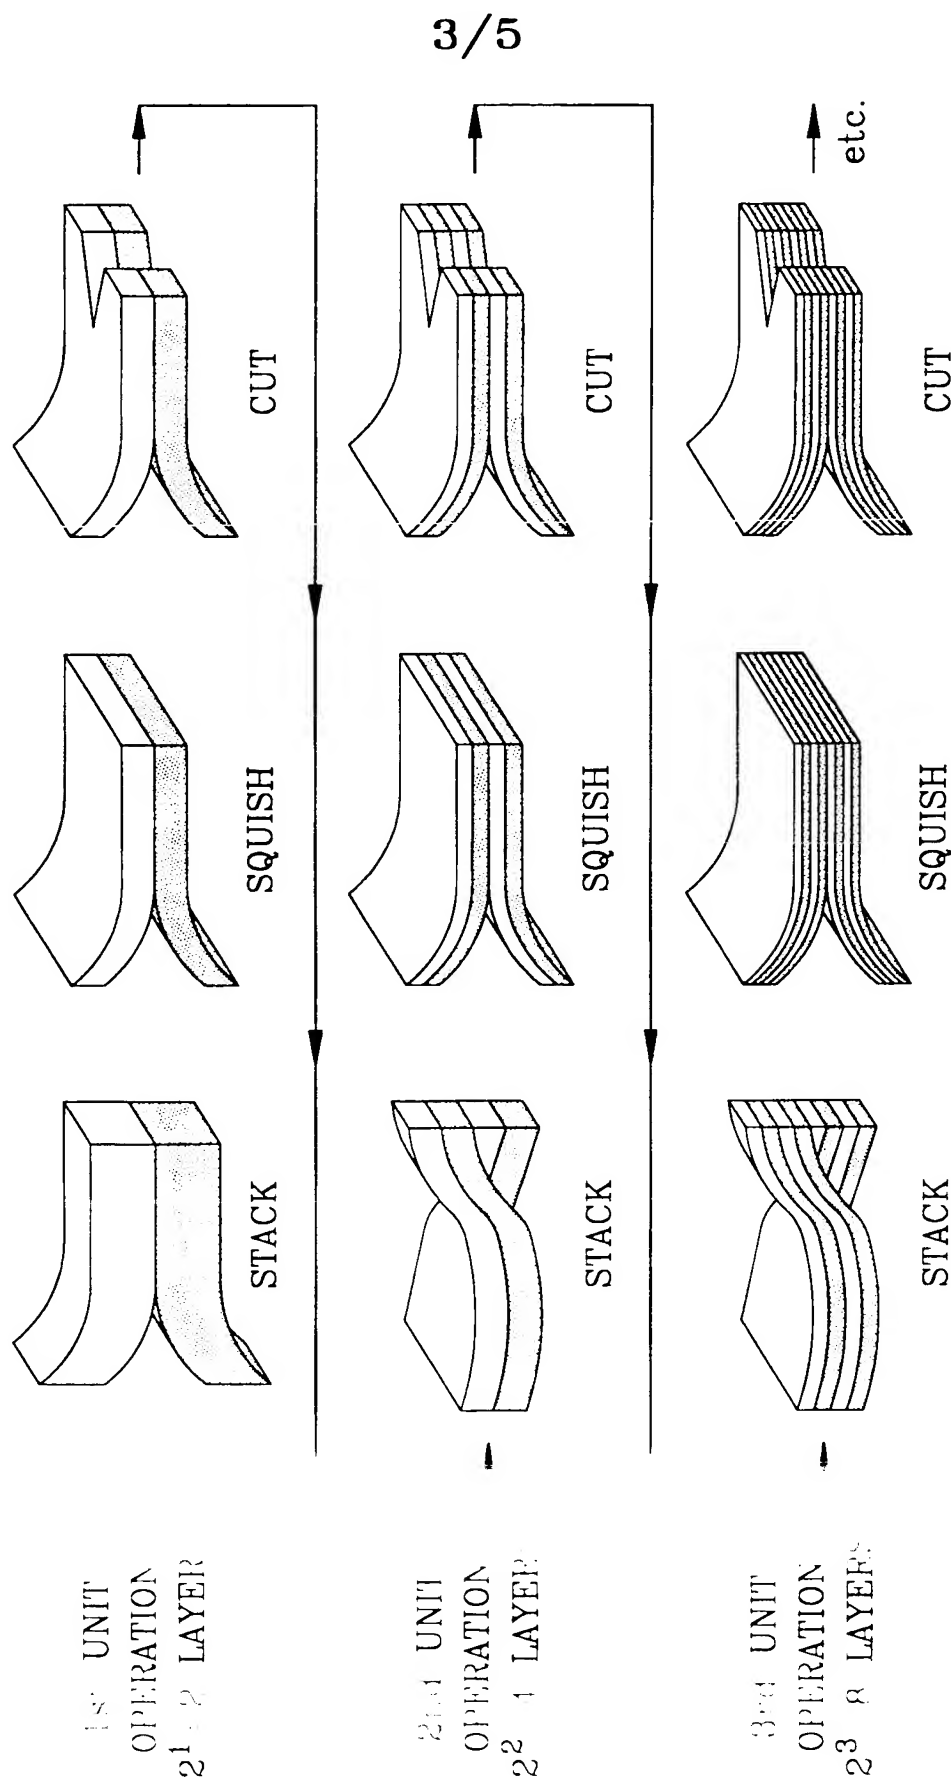


FIG-3

4/5

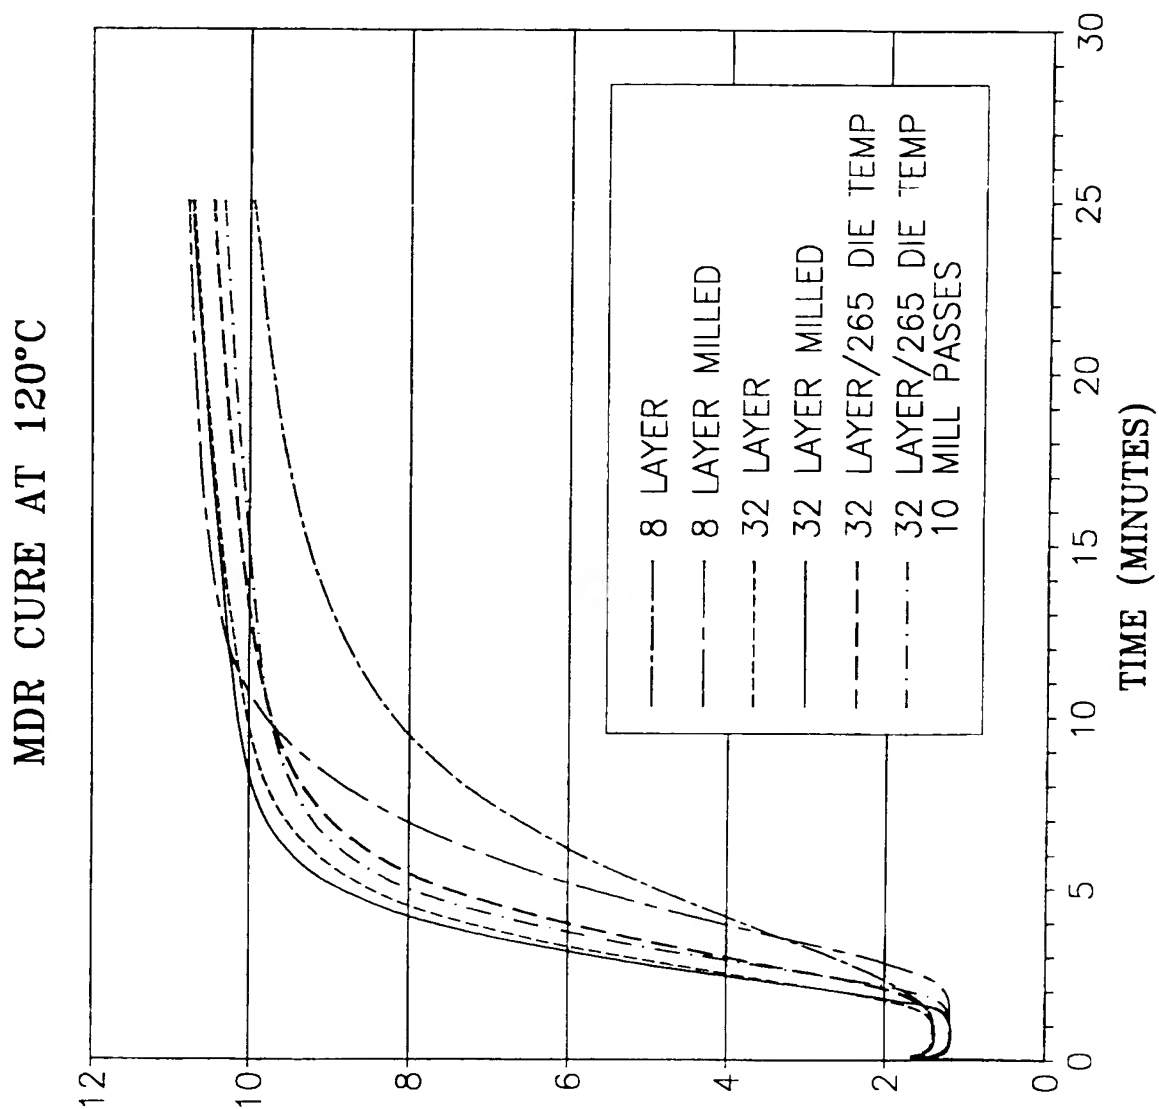


FIG-4

5/5

# MDR CURE AT 135°C

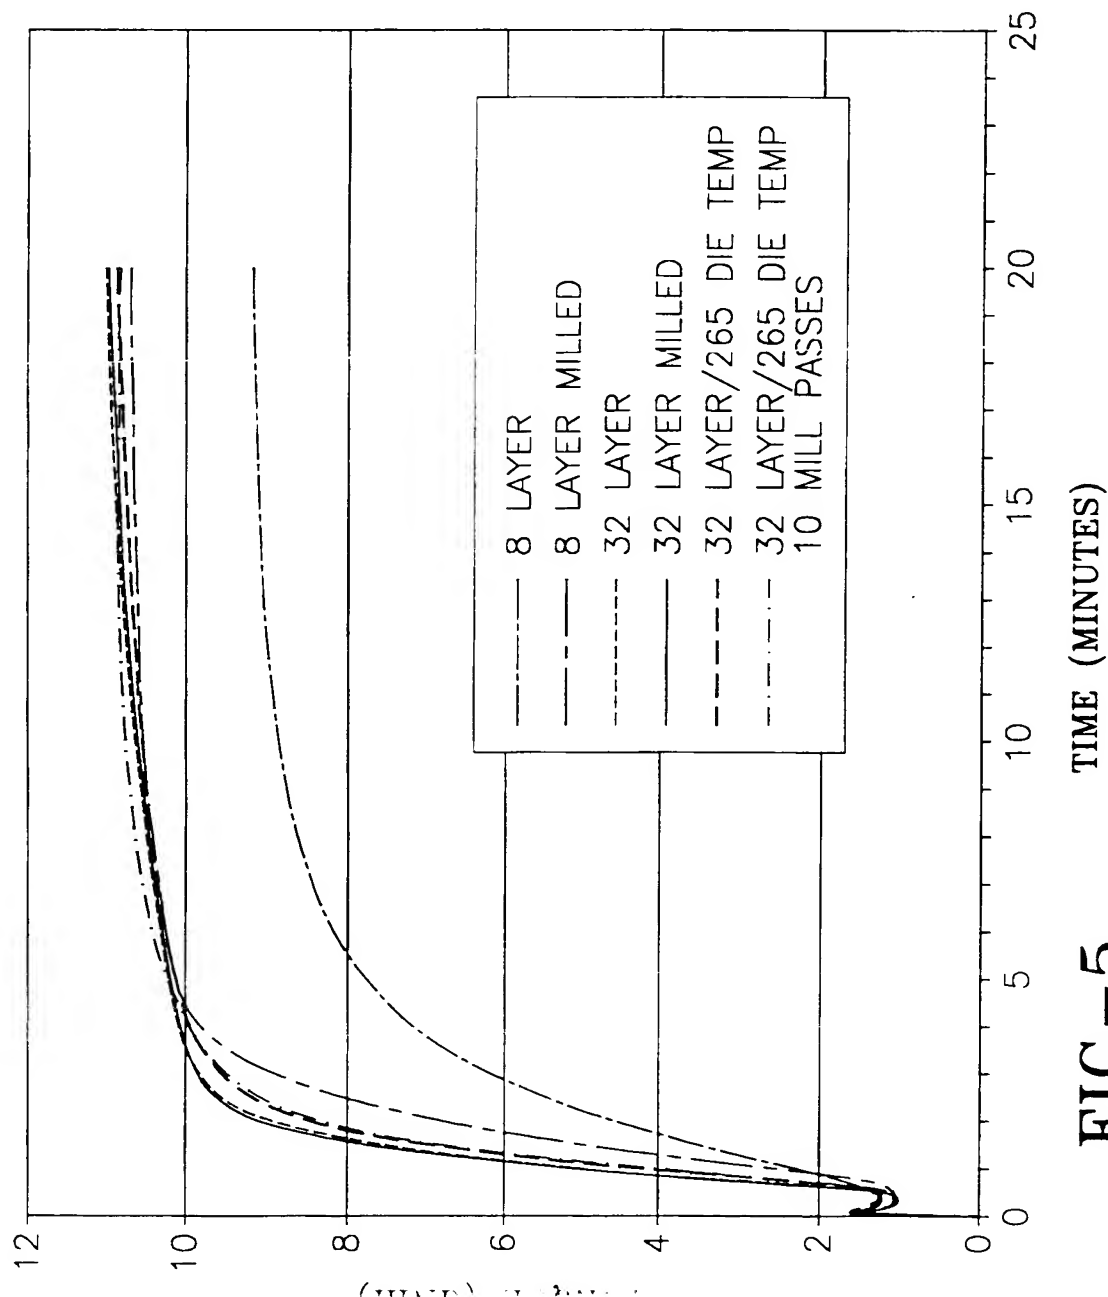


FIG-5